Canine Parvo Virus Antigen Test

For Veterinary Use Only

READ ALL INSTRUCTIONS BEFORE BEGINNING THE TEST

Introduction

Canine parvovirus (CPV), a nonenveloped single-stranded DNA (ssDNA) virus (family Parvoviridae, genus *Protoparvovirus*), is a highly successful pathogen that has sustained pandemic circulation in dogs for more than 40 years[1]. Canine parvoviruses are in the form of CPV-1 and CPV-2. Most dogs of CPV-1 infection are asymptomatic[2]. CPV-2 causes serious gastrointestinal and respiratory disease and has variants of CPV-2a, CPV-2b, and CPV-2c[3].

CPV enters through the mouth from the ground or floor and its incubation period is three to seven days before dogs appear symptoms[4]. CPV infected dogs appear lethargy, loss of appetite, abdominal bloating and pain, fever, or low body temperature (hypothermia), vomiting, and severe, often bloody, diarrhea[5].

Principle

The B!SAF CPV Ag Test Kit is a lateral flow chromatographic immunoassay for the qualitative detection of CPV antigens in canine feces. This kit shows two letters which are the test (T) line and the control (C) line on the surface of the device. If the CPV antigen exists in the sample, it binds to the gold-conjugated CPV antibody. The antigen-antibody complex moves through the membrane by capillary force and responds to the CPV antibody on the test line, resulting in a red line. The control line indicates that the test is performed correctly and should appear when the test is complete.

The highly selective and sensitive monoclonal antibody to CPV is used as a capture and detector in the kit. The B!SAF CPV Ag Test Kit can detect CPV antigen in canine feces with high accuracy.

Performance

1. Sensitivity & Specificity

		PCR		
		+	-	Total
CPV Ag Test	+	101	0	101
	-	2	214	216
	Total	103	214	317

Sensitivity: 98.06% (101/103, 95% CI*: 93.19% ~ 99.47%)

Specificity: 100% (214/214, 95% CI: 98.24% ~ 100%)

Diagnostic Agreement: 99.37% (315/317, 95% CI: 97.73% ~ 99.83%)

* CI: Confidence Interval

2. Limit of Detection: 5 x 10^3 $TCID_{50}$/mL

3. CPV-2, CPV-2a, CPV-2b diagnosis are also available.

4. Cross-Reactivity

Potentially cross-reactive substances listed below have no effect on the performance of the B!SAF CPV Ag Test Kit.

Pathogen	Titer	Result
Canine coronavirus	1.00 x 10^6 $TCID_{50}$/mL	Negative
Canine distemper virus	1.00 x 10^5 $TCID_{50}$/mL	Negative
Canine influenza virus	1.00 x 10^6 EID_{50}/mL	Negative
Escherichia coli	3.56 x 10^8 CFU/mL	Negative
Giardia spp.	1.42 x 10^5 Cysts/μL	Negative
Salmonella spp.	1.00 x 10^6 CFU/mL	Negative

Kit Components

Component	Quantity/kit by
1 CPV Ag test device	1
2 Dilution buffer	1
3 Disposable swab	1
4 Instructions for use	1
5 Collecrion bag	1

Storage & Stability

- Store in a dry place at 2-30°C
- Do not freeze
- Keep away from direct sunlight
- 24 months of shelf life (Production date to the expiration date).

Sample Preparation

1. Canine fecal swab should be used for this test.
2. The samples should be tested immediately after collection.
3. If samples cannot be tested immediately, they should be stored at 2~8°C (35.6~46.4°F) for up to 24 hours. For longer storage, freeze at -20°C (-4°F) or below. Frozen samples should be brought to room temperature (15~30°C/59~86°F) before use.
4. The amount of fecal sample with swab may affect the results. It is required to follow the swab amount of feces as shown in the picture below. The excessive fecal amount may induce a false positive result and slow migration.

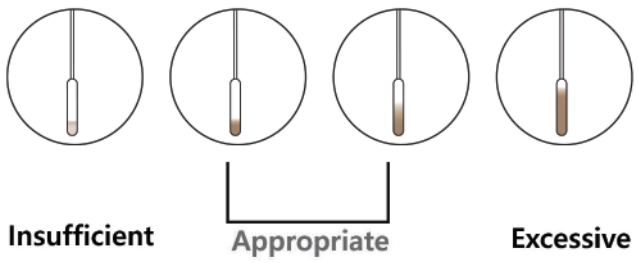

Test Procedure

1.All reagents and samples must be at room temperature (15~30°C/59~86 °F) before use.
2. Collect fecal sample using a swab.
3.Put the swab into the sample dilution buffer and stir the solution with the swab to disperse the sample into the buffer (approximately 10 seconds).
4.Wait for 2 minutes to settle down the large particles
5.Remove the swab from the sample dilution buffer.
6. Remove the test device from the pouch and place it on a flat and drysurface.
7.Apply 3 drops of the mixed sample solution into the sample holes foreach , drop by drop vertically.
8.Read test results at 10 minutes.

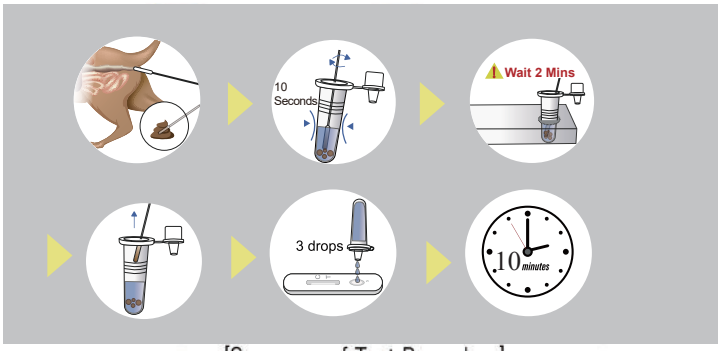

[Summary of Test Procedure]

Interpretation of Results

Positive(+)
Presence of two color bands "T"and "C"

Two lines, one nextto C and one next to T, even faint lines, shows the test is positive.



Negative (-)
No presence of color band ("T")

One red-coloredline only next to "C" indicates a negative result.

Invalid
No presence of color band ("C")

If the red-colored line in the control region "C" is not visible, the result is invalid. Run a new test.



Precautions

1. This test kit is for veterinary *in vitro* diagnostic use only for dogs. Do not use this test kit for other animals.
2. The test device is sensitive to humidity and heat. Use the test device within 10 minutes after removing the foil pouch.
3. Do not touch the membrane of the test device.
4. Do not use the test device if the foil pouch is damaged or the seal is open.
5. Do not use an expired test kit. The expiration date is marked on the package label.
6. Do not reuse the components (device, buffer, dropper, and swab).
7. Do not mix components from different lot numbers because the components in this kit have been quality control tested as a standard batch unit.
8. Decontaminate and dispose of all samples, used kits, and potentially contaminated materials in the accordance with national and local regulations.
9. All samples should be handled as being potentially infectious. Wear protective gloves while handling samples. Wash hands thoroughly afterward.

References

1. Voorhees IEH, Lee H, Allison AB, Lopez-Astacio R, Goodman LB, Oyesola OO, Omobowale O, Fagbohun O, Dubovi E, Hafenstein S, Holmes EC, Parrish CR. Limited Intrahost Diversity and Background Evolution Accompany 40 Years of Canine Parvovirus Host Adaptation and Spread. *J Virol.* 2020; 94(1): 1162-19.
2. Goddard A, Leisewitz AL. Canine Parvovirus. Veterinary Clinics of North America. *Small Animal Practice* 2010; 40(6): 1041-1053.
3. Cavalli A, Martella V, Desario C, Camero M, Bellacicco AL, Palo P, Decaro N, Elia G, Buonavoglia C. Evaluation of the Antigenic Relationships among Canine Parvovirus Type 2 Variants. *Clin Vaccine Immunol.* 2008; 15(3): 534-539.
4. Nandi S, Kumar M. Canine Parvovirus: Current Perspective Indian. *J Virol.* 2010; 21(1): 31-44.
5. Meunier PC, Cooper BJ, Appel MJ, Slauson DO. Pathogenesis of canine parvovirus enteritis: the importance of viremia. *Vet Pathol.* 1985; 22(1): 60-71.

Symbol Descriptions

LIC	License number
CAT	Catalogue number
LOT	Batch code, Lot number
	Consult instructions for use
Σn	Contains sufficient for ⟨n⟩ tests
	Do not reuse
IVD	*In vitro* diagnostic medical device
	Temperature limitation
	Do not use, if the package is damaged
	Upper side
	Manufacturer

Manufacturer: Feng Chun Yuan Medical Equipment(Shenzhen)Co.,Ltd
Address: Room.1304 & Room.1306 , No.48, Xinyu Road, Xiangshan Community Xinqiao Street, Baoan District, Shenzhen, Guangdong, China. 518 000

EC REP Riomavix S.L.
Add.: Calle de Almansa 55, 1D, Madrid 28039 Spain
Tel.: +34 658 396 230
E-mail: leis@riomavix.com

Importer & Distributor: BISAF Sp. z o.o.
Add: ul. Rdestowa 5, 54-530 Wrocław, Poland
Website: www.bisaf.pl